


Synchrony II Ventilator

A Quick Guide


1. Plug in and Switch on (remember this ventilator has no internal Battery)

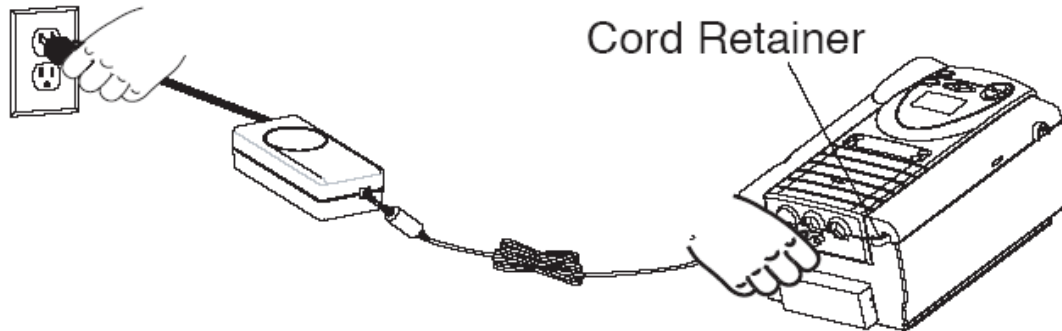


2. Apply Mask to patient



3. Attach Circuit to ventilator

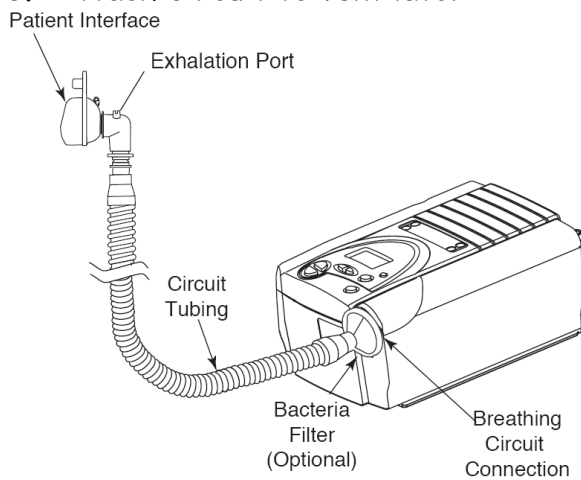


4. Turn Blower on

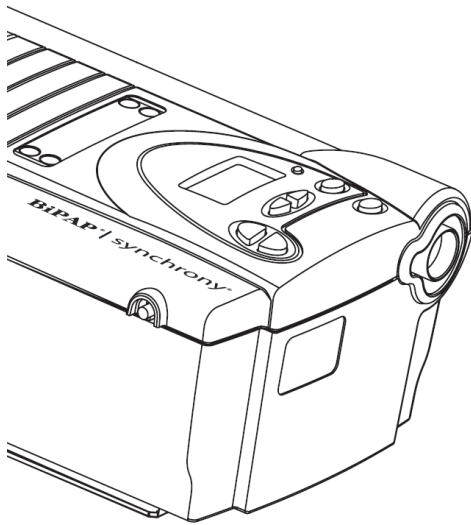


5. Attach Circuit to Mask

6. Check Pressure Reading - see ventilator data sheet

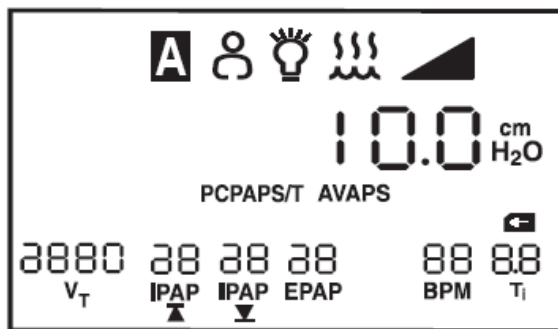

7. Check exhalation port is working

8. The only alarm is the Disconnect Alarm and this is set at 15 or 60 seconds

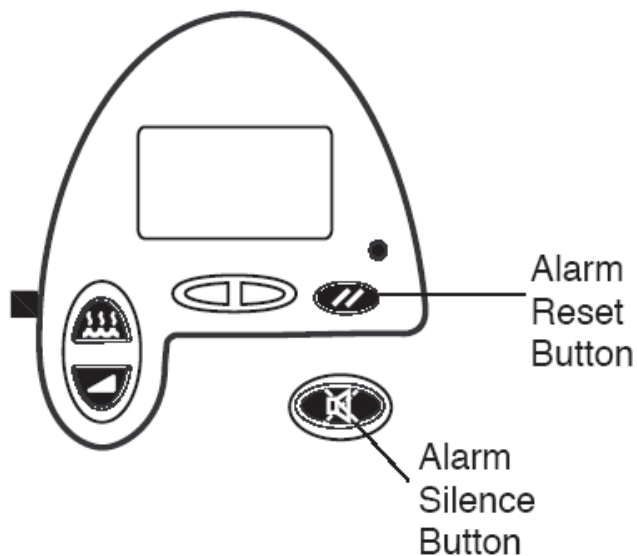

9. If Vent Fails, take it OFF and seek help in the morning